
STILLE imagiQ3™ Legacy
Unparking instructions

Surgical perfection. For life.


The imagiQ3 Legacy is a **mobile** imaging table.
It can be moved with or without patient.

In order to unpark the table, it must be in **Safe Position**. The table will beep and not allow unparking if it is not in Safe Position. To achieve “Safe Position“, follow these steps:



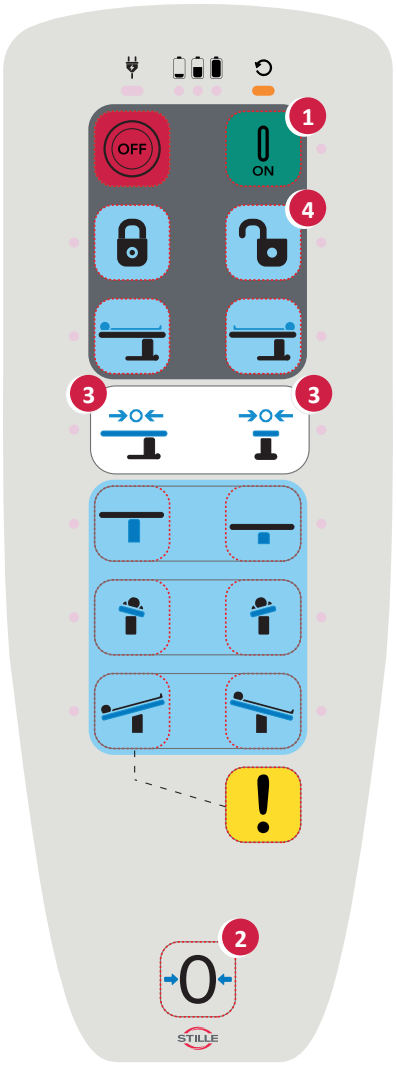


1 **Turn the hand control ON**
by pressing the GREEN button.



2 **Press and hold the “0“ button**
which will level the table.



3 **Center the tabletop**
by pressing down the mushroom Pan Handle and moving the tabletop to the center. The tabletop is correctly centered when both LED lights on the hand control are illuminated. This is the Safe Position.



4 **Press and hold the unlock button**
until the unpark LED stays lit. The table can now be moved on its wheels.

STILLE
Surgical perfection. For life.

STILLE - Service Centers

STILLE AB
Ekbacken 11
SE-644 30 Torshälla
Sweden
+46 8 588 580 00
service@stille.se
www.stille.se

STILLE Surgical Inc.
840 Parkview Blvd
Lombard, IL 60148
United States
1.800.665.1614
service.us@stille.se
www.stille.se/us

Doc ID: 953-G550-0007-EN-01 imagiQ3™ Legacy Unparking Instructions © 2025-05-08 STILLE. All rights reserved.